


## Selecting a Bioamplifier for Single - Subject Recordings

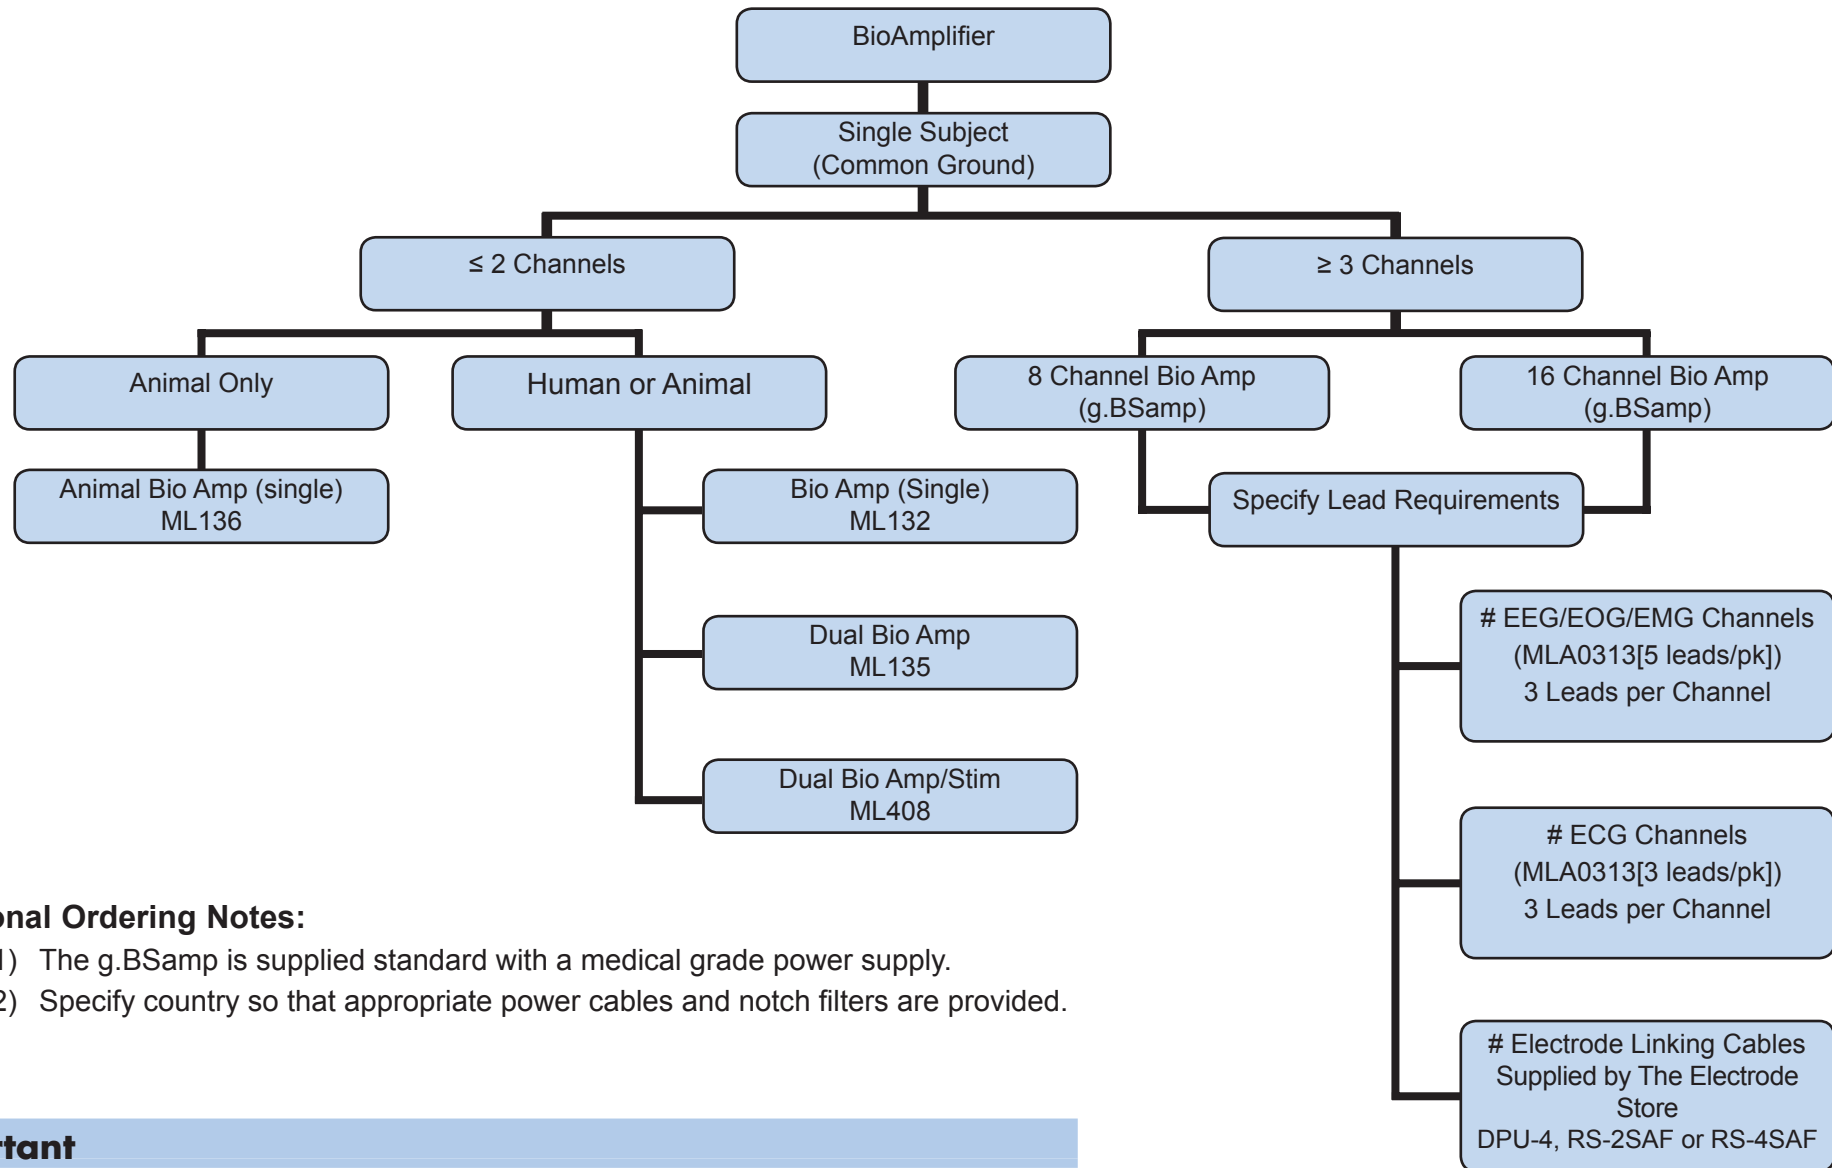

### Additional Ordering Notes:

- 1) The g.BSamp is supplied standard with a medical grade power supply.
- 2) Specify country so that appropriate power cables and notch filters are provided.

### Important

If you wish to record biopotentials from multiple subjects, please contact your local ADInstruments representative for further information.